

Reviewing the use of chitosan and polydopamine for electrochemical sensing

Citation for published version (APA):

Prabhu, A., Crapnell, R. D., Eersels, K., van Grinsven, B., Kunhiraman, A. K., Singla, P., McClements, J., Banks, C. E., Novakovic, K., & Peeters, M. (2022). Reviewing the use of chitosan and polydopamine for electrochemical sensing. *Current Opinion in Electrochemistry*, 32, Article 100885. <https://doi.org/10.1016/j.coelec.2021.100885>

Document status and date:

Published: 01/04/2022

DOI:

[10.1016/j.coelec.2021.100885](https://doi.org/10.1016/j.coelec.2021.100885)

Document Version:

Publisher's PDF, also known as Version of record

Document license:

Taverne

Please check the document version of this publication:

- A submitted manuscript is the version of the article upon submission and before peer-review. There can be important differences between the submitted version and the official published version of record. People interested in the research are advised to contact the author for the final version of the publication, or visit the DOI to the publisher's website.
- The final author version and the galley proof are versions of the publication after peer review.
- The final published version features the final layout of the paper including the volume, issue and page numbers.

[Link to publication](#)

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal.

If the publication is distributed under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license above, please follow below link for the End User Agreement:

www.umlib.nl/taverne-license

Take down policy

If you believe that this document breaches copyright please contact us at:

repository@maastrichtuniversity.nl

providing details and we will investigate your claim.

Review Article

Reviewing the use of chitosan and polydopamine for electrochemical sensing

Akash Prabhu¹, Robert D. Crapnell², Kasper Eersels³,
 Bart van Grinsven³, Aruna K. Kunhiraman¹, Pankaj Singla⁴,
 Jake McClements⁴, Craig E. Banks², Katarina Novakovic⁴ and
 Marloes Peeters⁴



Abstract

Biopolymers possess highly favorable properties for electrochemical biosensing such as their inherent biocompatibility, inexpensive nature, and strong interfacial adhesion. In this mini-review, we will focus on chitosan and polydopamine, two of the most commonly used biopolymers, for electrochemical sensing applications. Chitosan is a polysaccharide that exhibits high chemical resistance, offers straightforward modification and cross-linking, and possesses antibacterial properties and mucoadhesion. Polydopamine has the benefit of universal adhesion, in addition to the ability to form self-assembled structures. We will demonstrate how the unique structural and electrochemical features of these biopolymers can be used in a range of electrochemical biosensing platforms.

Addresses

¹ Rathinam Technical Campus, Rathinam Techzone, Pollachi Rd, Eachanari, Tamil Nadu, 641021, India

² Manchester Metropolitan University, Faculty of Science and Engineering, Chester Street, M1 5GD, Manchester, UK

³ Maastricht University, Faculty of Science and Engineering, Sensor Engineering Department, PO Box 616, 6200 MD Maastricht, the Netherlands

⁴ Newcastle University, School of Engineering, Merz Court, Claremont Road, NE1 7RU, Newcastle Upon Tyne, UK

Corresponding author: Peeters, Marloes (marloes.peeters@ncl.ac.uk)

Current Opinion in Electrochemistry 2022, 32:100885

This review comes from a themed issue on **Sensors and Biosensors**

Edited by **Luís Moreira Gonçalves**

For complete overview about the section, refer [Sensors and Biosensors 2022](#)

Available online 17 November 2021

<https://doi.org/10.1016/j.coelec.2021.100885>

2451-9103/© 2021 Elsevier B.V. All rights reserved.

Keywords

Biopolymer, Chitosan, Polydopamine, Biosensors, Electrochemistry,
 Electrochemical sensing.

Introduction

International Union of Pure and Applied Chemistry (IUPAC) defines biopolymers as macromolecules,


including proteins, nucleic acids, and polysaccharides, that are formed by living organisms [1]. Generally, biopolymers can be divided into three classes depending on their monomer units: polynucleotides; polypeptides; and polysaccharides [2]. Considering the exponential surge in plastic waste, it is expected that biopolymers, especially those available from waste material, will play an important role in future-proofing advanced materials including advanced electrochemical sensors [3]. The focus of this mini-review will be on chitosan and polydopamine (PDA), two of the most commonly used biopolymers, which promote sustainability as they are nontoxic and can be produced via ‘green chemical’ synthesis routes. The focus of this minireview will be on chitosan and PDA, two of the most commonly used biopolymers, which promote sustainability as they are non-toxic and can be produced via “green chemical” synthesis routes. However, there are significant barriers to implementation of these materials including costs, conductivity, and reproducibility, which is why they are not routinely used in electrochemical sensors. The review outlines challenges in the field as a result of the growing use of electrochemical sensors for *in vitro* and *in vivo* detection and highlights the foreseen next generation of hybrid biopolymer materials which have potential to overcome current shortcomings.

Chitosan

Chitosan is commercially produced from the biopolymer chitin because it is only naturally found in small quantities in some fungi. It is a partially, or to a significant extent, deacetylated derivative of chitin (Figure 1), which is the second most abundant polysaccharide in nature after cellulose and is found in cell walls of green algae, insect cuticles, and crustacean exoskeletons [4].

The number of monosaccharides in chitosan can vary quite significantly, leading to large variations in the degree of deacetylation, molecular weight, and pKa values of even commercial batches, which complicates reproducibility of the material. Chitosan has two reactive groups, a primary amine and hydroxy on the glycosidic residue, which can be used for side group attachment

Figure 1

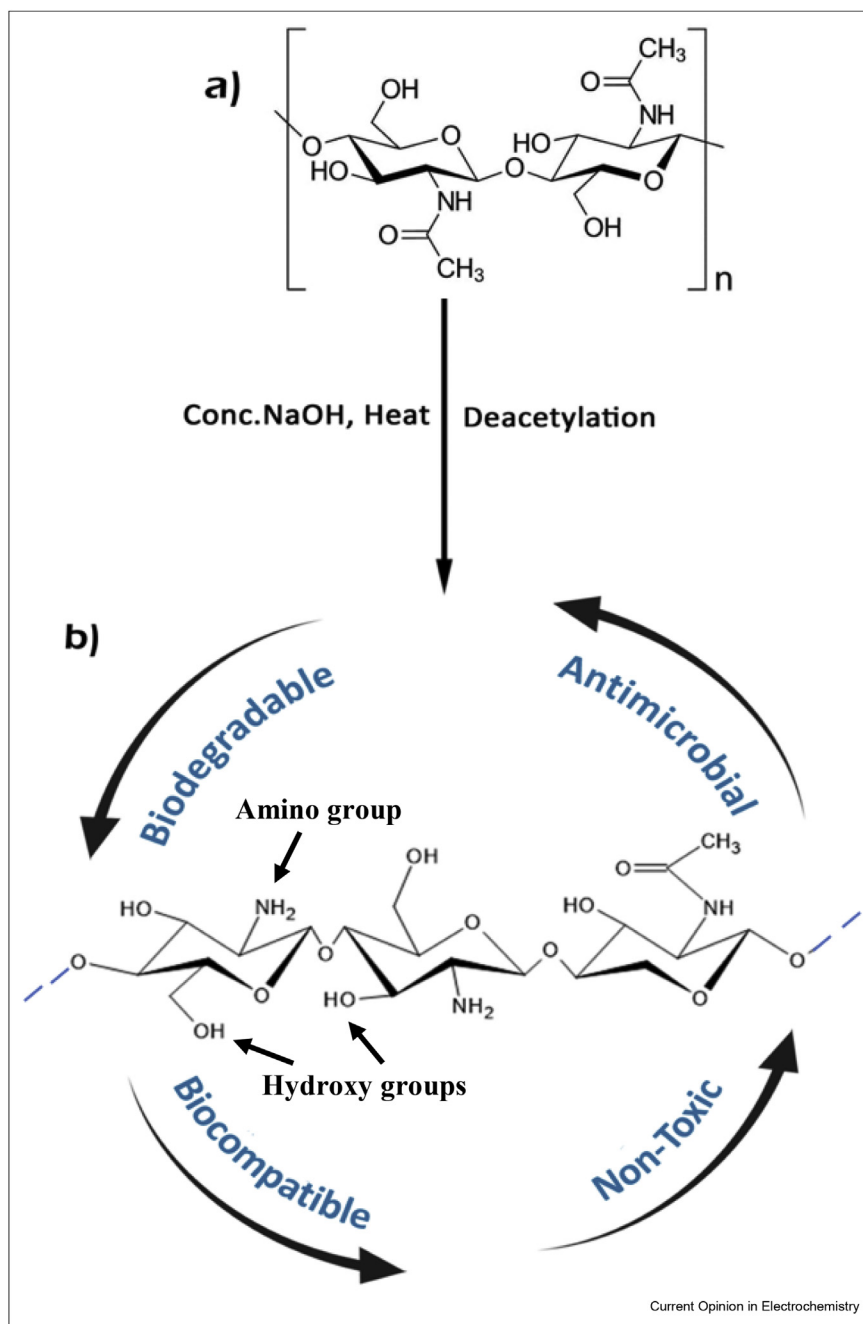

Formation of chitosan: (partial) deacetylation of chitin (a) into chitosan (b) where the dashed lines represent continuation of the structure.

[5]. These groups are strongly pH-dependent, and therefore have excellent applications in drug delivery but can lead to complications with electrostatic repulsion under specific conditions [6]. Generally, chitosan is cross-linked to improve susceptibility to mechanical and physiochemical damage; these cross-linked materials may exhibit new properties, such as fluorescence while retaining their own critical characteristics [7].

Polydopamine

PDA is a dark brown biopolymer produced by autoxidation of dopamine, which is also a synthetic analog of naturally occurring melanin (a pigment) [8]. PDA's chemical structure is rich in functional groups such as catechol, amine, and imines [Figure 2]. The favorable adhesive properties of the compound are attributed to different chemical reactions and interaction

mechanisms with the catechol group such as Michael-type addition, Schiff base reactions, and hydrogen bonding [9]. Although the catechol group plays a key role in adhesive properties, the other functional groups make PDA a versatile material with applications in different areas such as sensing [10].

Sensing applications

Chitosan-based sensors

Chitosan can be produced as three-dimensional structures, brushes, or thin films using various approaches including electrodeposition and drop-casting [11–13]. The material can have various functions in sensors such as serving as a matrix material, improving dispersion because of its hydrophilic nature, and guaranteeing selectivity by forming noncovalent bonds [14]. As a three-dimensional network, chitosan has a very large surface area, in addition to good structural and chemical stability, which makes it highly suitable for the impregnation of recognition elements.


For example, a chitosan/polyaniline-gold nanocomposite was deposited onto tin oxide-coated glass plates for the detection of cholesterol using cholesterol oxidase enzymes [15]. This voltammetric sensor exhibited a linear range from 50 to 500 mg/dL, with a shelf-life of three weeks. An example of a chitosan/graphene-based sensor is shown in Figure 3, where detection of chromium VI was possible in a wide linear range (10^{-5} – 10^{-9} mol/L) using differential pulse voltammetry, which generally is the electrochemical sensing strategy with the highest specificity [16*].

There is also considerable interest in incorporating antibodies into chitosan because traditional matrices composed of inorganic nanomaterials are hydrophobic,

which can lead to low/heterogeneous surface coverage. Recently, research has focused on comixture nanomaterials by using chitosan's ability to interlink with other materials [17]. However, the use of biological elements such as antibodies and enzymes has the disadvantage of limited stability in extreme environments (e.g. high temperatures), and immobilization of recognition elements is not always straightforward. Molecularly imprinted polymers (MIPs), porous materials containing high-affinity binding sites to a specific target, present an interesting alternative. A comprehensive review of MIPs based on chitosan is provided in the study reported by Zouaoui *et al.* [18**]. The most promising approach to achieve a controlled structure of porous chitosan in MIP-based sensors is by electrodeposition. In short, electrodeposition can be achieved by immersing a working electrode into a chitosan solution (deposition solution) followed by application of the desired voltage (typically -1.5 V) for a fixed amount of time [11]. At this potential, the amine group of chitosan becomes a cationic polyelectrolyte, and the positively charged molecule of the polymer is attracted toward the negatively charged cathode. Because the electrochemical performance of these films is hampered by chitosan's poor electrical conductivity, it is vital to include nanomaterials to improve electron transfer. These can be inorganic materials or conductive polymers because chitosan can form hybrids through conjugated π -bonds with polypyrrole and polyaniline [19].


Chitosan can also be applied as brushes, and layer-by-layer grafting techniques have been used to deposit chitosan onto metal alloys to make them suitable as implant materials [20]. PDA surface modification can be used in this process because it is used as a strong adhesive in various environments and improves the overall

Figure 2

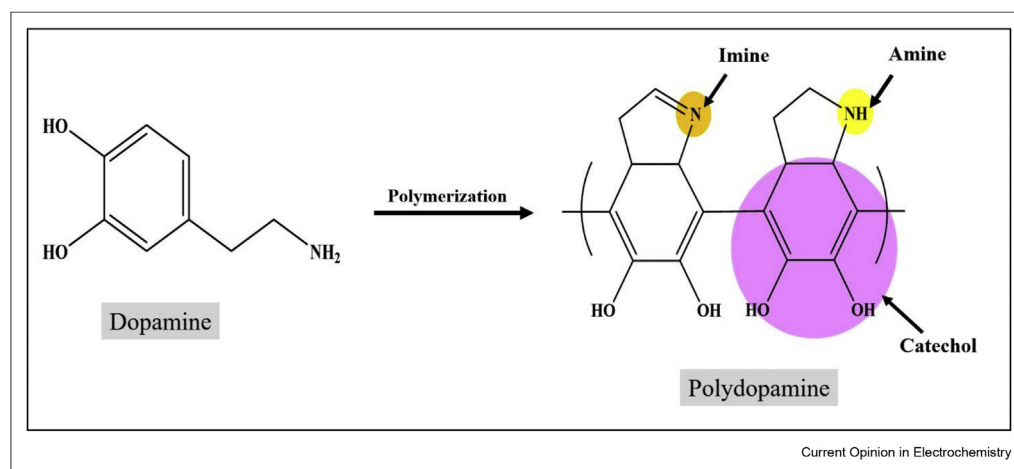

Polymerization reaction of dopamine. The arrows indicate functional groups on the polymer, such as the imine, amine, and catechol.

Figure 3

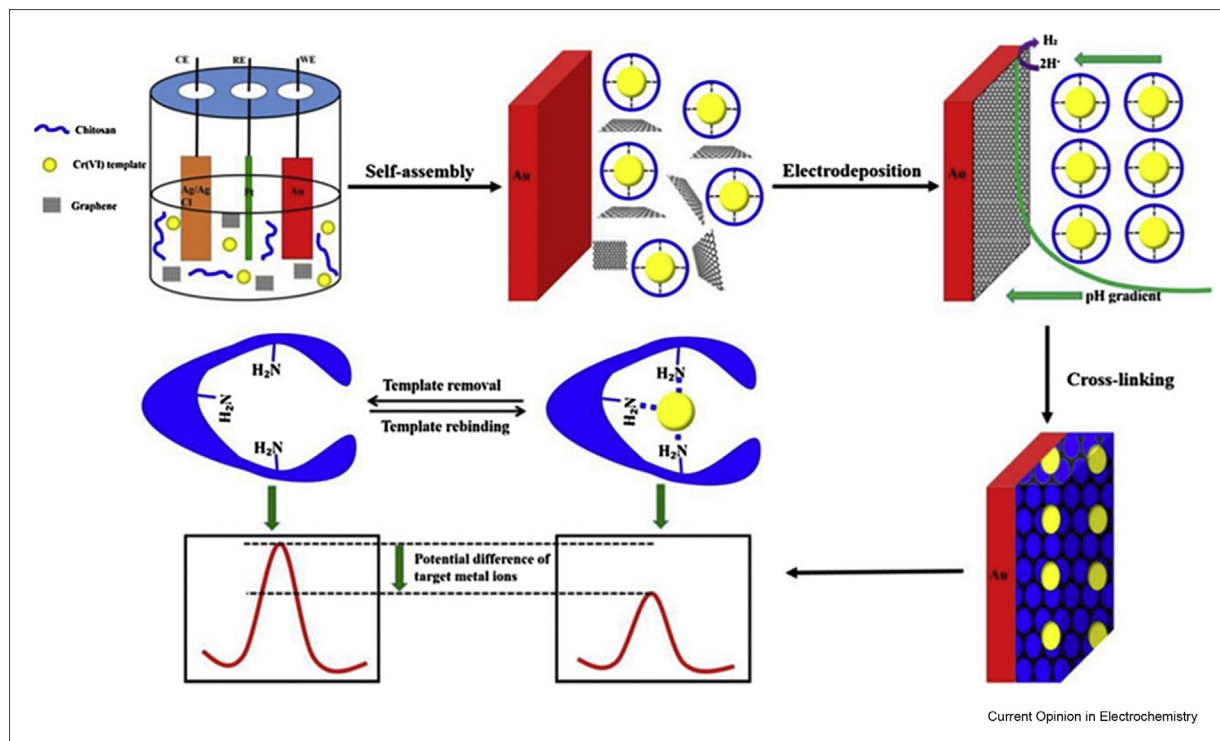

Electrodeposition of graphene/chitosan constructs onto electrodes in the presence of a Cr (VI) template. After washing the surface, binding sites are formed, and rebinding of the template leads to a distinct change in the DPV signal [16^{*}]. Reprinted with permission from Elsevier. DPV, differential pulse voltammetry.

stability of the system [21]. Wang et al. [12], developed a high-performance electrochemical sensor for hydroquinone and catechol by using the advantageous properties of multiwalled carbon nanotubes (surface area), PDA (conductivity), and chitosan (selective detection). These brushes can also be combined with biomimetic recognition elements such as aptamers. A rapid electrochemical sensor for *Listeria monocytogenes* was developed using chitosan-aptamer nanobrushes that could detect the microorganism of interest without preconcentration, even in the presence of other Gram-positive cells [22]. The high selectivity of brush borders in natural systems was the inspiration for this article; compared with traditional stimulus materials such as poly (N-isopropyl acrylamide) and ionic polymer-metal composites, chitosan is the most attractive for analysis of food samples owing to its low cost and biocompatibility [23]. However, challenges with this approach mainly stem from the fact that chitosan exhibits pH-dependent behavior, which impedes detection in real samples.


PDA-based sensors

PDA's popularity for electrochemical sensing applications stems from their structure and functional groups, which lead to the formation of strong affinities

with a plethora of solid surfaces, intrinsic chemical reactivity with nucleophiles, ability to chelate metal ions, and redox activity [24]. The thickness of PDA films deposited using alkaline oxygenated solutions can be controlled by varying the concentration of dopamine monomer, which can also affect the surface morphology of the film [25]. These systems must be carefully designed as many features of PDA formation and structure remain unknown, and the intrinsic chemical reactivity of the PDA toward nucleophiles is spontaneous [26^{**}]. In addition, a well adhered, full coverage of PDA on an electrode surface is undesirable in many electrochemical applications owing to fouling of the electrode. The full mechanism of PDA formation remains unclear, with it expected to be a 2-electro 2 proton transfer process. However, there are a plethora of after oxidation reactions that can occur depending on the electrode surface that can lead to the formation of compounds that inhibit electron transfer.

PDA nanospheres present an alternative to surface modification and can be formed through stirring in alkaline media [27]. This offers the ability to control PDA nanosphere size, use functional groups to form linkages or anchors to other structures through covalent

Figure 4

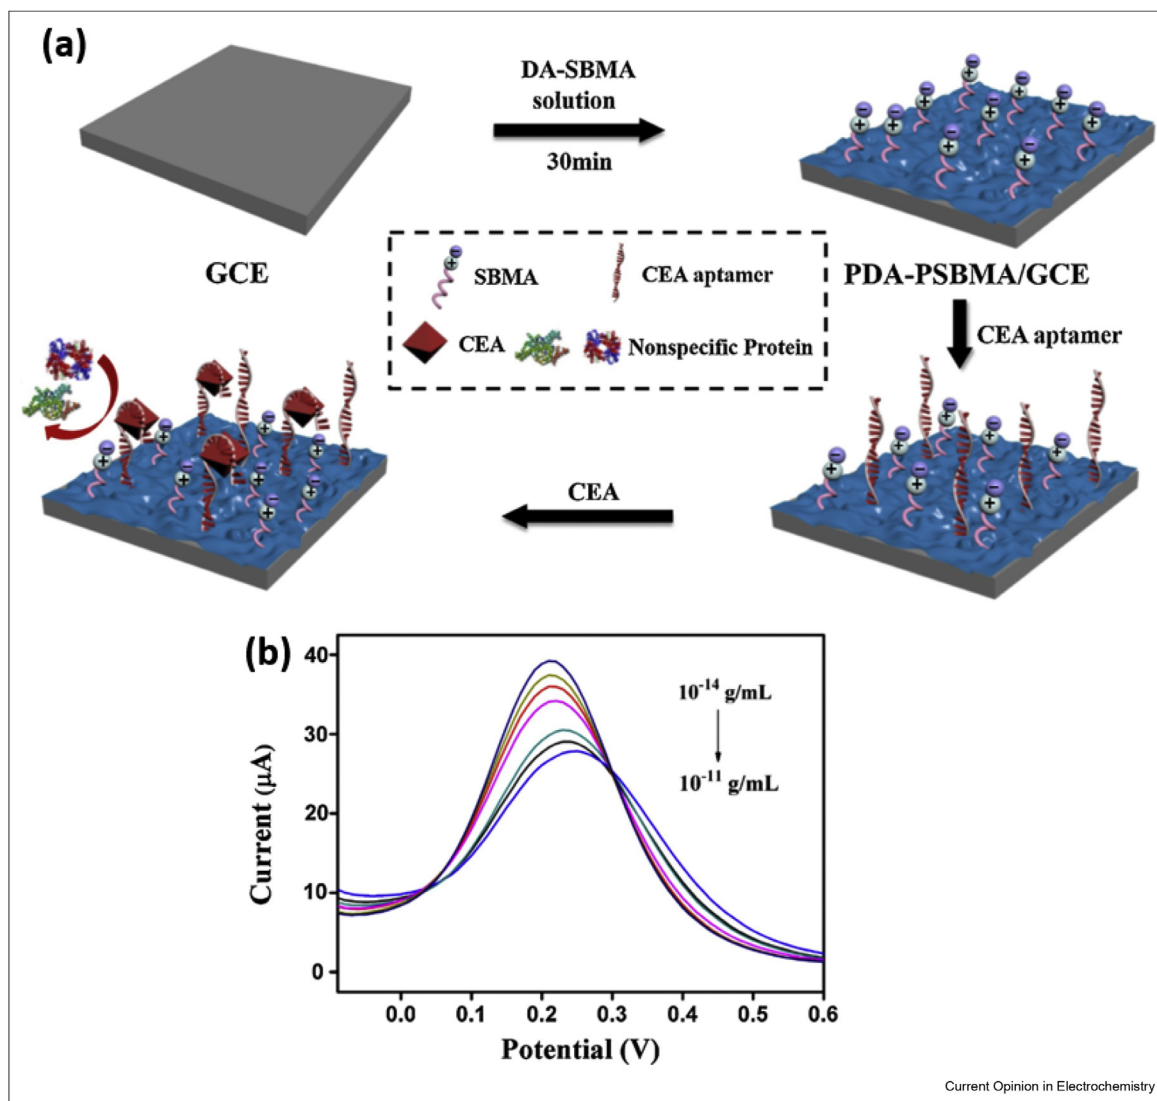

PDA-PSBMA sensor fabrication. (a) Illustration of the PDA-PSBMA-based sensor's fabrication. (b) DPV response to increasing concentrations of CEA. Modified with permission from Elsevier, see the study reported by Xu *et al.* [42^{*}]. CEA, carcinoembryonic antigen; DPV, differential pulse voltammetry; PDA, polydopamine; PSBMA, poly(sulfobetaine methacrylate).

bonding, and even form self-assembled monolayers on surfaces for sensing applications [28,29].

The ability to form a multifunctional surface can be used in conjunction with nanomaterials to enhance the electrochemical biosensing capabilities of different platforms [30]. Liu *et al.* [31] demonstrated this through the use of PDA-coated reduced graphene oxide as a base for the formation of an *o*-phenylenediamine MIP film for the detection of 2,4-dichlorophenol using differential pulse voltammetry. PDA can also be used as the MIP itself, the presence of catechol and amine functional groups and their ability to form strong noncovalent interactions with target molecules and proteins have given rise to the popularity of using

dopamine as the functional monomer. Through spontaneous alkaline aqueous oxidation, these MIPs can be incorporated into biosensing platforms in various forms such as hollow MIPs and magnetic MIPs [32,33]. Alternatively, PDA MIPs can be formed through electropolymerization of the dopamine monomer [34,35]. One of the first examples by Liu *et al.* [36] used cyclic voltammetry in a deoxygenated solution of dopamine in the presence of their target nicotine, creating a compact, insulating film.

Tretjakov *et al.* [37] used a surface linker to immobilize their target before polymerization. They designed PDA films of specific thicknesses via electrodeposition and compared their performance for the detection of

immunoglobulin G, achieving the best imprinting effect with a film thickness of 17 nm. The formation of MIPs for large targets can be hindered by the formation of PDA as it is kinetically driven and has a saturation limit of less than 50 nm owing to dopamine depletion, although we note PDA layers can be deposited onto pre-existing layers [26*]. Kanyong et al. [38] electro-polymerized dopamine hydrochloride onto a screen-printed carbon electrode (SPCE) through cyclic voltammetry to form the PDA-SPCE. This modified electrode produced well-defined redox peaks when scanned in Britton–Robinson buffer. Proof-of-concept application for the detection of biomolecules was achieved using guanine in which a 5-fold increase in anodic peak current was observed when using the PDA-SPCE.

Finally, PDA can also be incorporated with other polymers on electrode surfaces to produce electrochemical sensing platforms [39]. Salgado et al. [40] used electrochemical techniques to prepare poly (3,4-ethylenedioxythiophene) nanowires onto Pt surfaces modified with PDA. Research into the copolymerization of PDA for electrochemical sensor platforms has also been reported recently with polypyrrole to increase film conductivity [41]. This work used the functional groups of PDA to facilitate adhesion between a zwitterionic polymer with antifouling properties to aptamer recognition elements for selective detection. Another recent study by Xu et al. developed an electrochemical biosensor for the tumor biomarker carcinoembryonic antigen using copolymerized PDA and the zwitterionic polymer poly (sulfobetaine methacrylate). The polymers were deposited onto a glass carbon electrode and were able to detect the relevant target well within physiologically relevant range (~ 3 fg/mL) as illustrated in Figure 4.

Future work and outlook

The use of chitosan and PDA for biomedical applications is relatively new; chitosan was approved for medical use in the United States in 2003, and the first works on PDA for multifunctional coatings and its polymerization mechanism were published in 2007 [43*]. This means commercial products are limited, with no applications in electrochemical sensing to date. It is expected that a trend will emerge of increased use of these materials especially in hybrid form because they can bring unique properties (e.g. adhesion and biocompatibility) to sensors. Both materials will have challenges in terms of costs, and large-scale production is limited; therefore, incentives should be considered to promote the use of ‘green’ production of biopolymers to prevent further increase of plastic waste. However, the use of these materials in the future is prone to different challenges.

For chitosan, the main challenges are improving batch-to-batch variation to have access to medium to large-

scale industrial batches with reproducible properties and incorporation of materials to increase conductivity. As conductivity will remain an inherent problem, this biopolymer might find more applications in platforms using nonelectrochemical read-out techniques (thermal, optical, gravimetric detection, and so on). Alternatively, chitosan can be used as matrix material to improve the surface area or added to improve overall biocompatibility, although it has to be noted that not all structures of chitosan are biocompatible. Chitosan-based electrochemical sensors can also be explored for the detection of specific cells and combined with targeted drug delivery.

PDA is generally conductive; however, when coated onto electrodes, the conductivity of the electrode decreases, especially on microelectrodes that are typically required for *in-vivo* detection [44]. Care must be taken when developing electrochemical sensors using PDA owing to its inherent spontaneous chemical reactivity toward nucleophiles and possible interference from redox peaks depending on the layer thickness and morphology [45]. However, this reactivity is also its main benefit because it facilitates adhesion between different structures.

The biocompatibility of both materials in microstructures can be questioned. However, PDA and chitosan coatings on different nanoparticles generally ensure good physicochemical properties and biocompatibility, thus facilitating *in-vivo* biosensing, cell imaging, and detection of various diseases. In light of the above-mentioned advantages of chitosan and PDA, there is great potential for their further use in portable electrochemical devices if costs are reduced, and large-scale commercial production is achieved in the future.

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgements

The authors would like to acknowledge the European Commission for funding of salary of PS (grant TEMPER 893371) and the Rosetrees Trust for funding of salary of JMC (Seedcorn2020\100303).

References

Papers of particular interest, published within the period of review, have been highlighted as:

- * of special interest
- ** of outstanding interest

1. Nagel B, Dellweg H, Gierasch LM, Dellweg H, Engels JW, Fox JL, Gierasch LM, Gregson RP, Heinritz B, Leuenberger HGW, Moo-Young M, Moser A, Nagel B, Nyeste L, Pcnasse L, Petersen GB, Van Montagu M, Yamada Y: **Glossary for chemists of terms used in biotechnology**. *Pure Appl Chem* 1992, **64**:143–168, <https://doi.org/10.1351/pac199264010143>.

2. George A, Sanjay MR, Srisuk R, Parameswaranpillai J, Siengchin S: **A comprehensive review on chemical properties and applications of biopolymers and their composites.** *Int J Biol Macromol* 2020, **154**:329–338, <https://doi.org/10.1016/j.jbiomac.2020.03.120>.
 3. Vinod A, Sanjay MR, Suchart S, Jyotishkumar P: **Renewable and sustainable biobased materials: an assessment on biofibers, biofilms, biopolymers and biocomposites.** *J Clean Prod* 2020, **258**, 120978, <https://doi.org/10.1016/j.jclepro.2020.120978>.
 4. Alishahi AA: **Chitosan: a bioactive polysaccharide in marine-based foods.** In *The complex world of polysaccharides*. Edited by Karunaratne DN, Rijeka: Intech; 2012:409–428, <https://doi.org/10.5772/48199>.
 5. Tharanathan RN, Kittur FS: **Chitin - the undisputed biomolecule of great potential.** *Crit Rev Food Sci Nutr* 2003, **43**:61–87, <https://doi.org/10.1080/10408690390826455>.
 6. Vukajlovic D, Parker J, Bretcanu O, Novakovic K: **Chitosan based polymer/bioglass composites for tissue engineering applications.** *Mater Sci Eng C* 2019, **96**:955–967, <https://doi.org/10.1016/j.msec.2018.12.026>.
 7. Ryan C, Alcock E, Buttner F, Schmidt M, Clarke D, Pemble M, Bardosova M: **Synthesis and characterisation of cross-linked chitosan composites functionalised with silver and gold nanoparticles for antimicrobial applications.** *Sci Technol Adv Mater* 2017, **18**:528–540, <https://doi.org/10.1080/14686996.2017.1344929>.
 8. Batul R, Tamanna T, Khaliq A, Yu A: **Recent progress in the biomedical applications of polydopamine nanostructures.** *Biomater. Sci.* 2017, **5**:1204–1229, <https://doi.org/10.1039/c7bm00187h>.
 9. Ding YH, Floren M, Tan W: **Mussel-inspired polydopamine for bio-surface functionalization.** *Biosurface and Biotechnology* 2016, **2**:121–136, <https://doi.org/10.1016/j.bsbt.2016.11.001>.
 10. Liu Y, Ai K, Lu L: **Polydopamine and its derivative materials: synthesis and promising applications in energy, environmental, and biomedical fields.** *Chem Rev* 2014, **114**: 5057–5115, <https://doi.org/10.1021/cr400407a>.
 11. Liu J, Wang X, Wang T, Li D, Xi F, Wang J, Wang E: **Functionalization of monolithic and porous three-dimensional graphene by one-step chitosan electrodeposition for enzymatic biosensor.** *ACS Appl Mater Interfaces* 2014, **6**: 19997–20002, <https://doi.org/10.1021/am505547f>.
 12. Pavinatto A, de Almeida Mattos AV, Malpass ACG, Okura MH, Balogh DT, Sanfelice RC: **Coating with chitosan-based edible films for mechanical/biological protection of strawberries.** *Int J Biol Macromol* 2020, **151**:1004–1011, <https://doi.org/10.1016/j.jbiomac.2019.11.076>.
 13. Poletti F, Favaretto L, Kovtun A, Treossi E, Corticelli F, Gazzano M, Palermo V, Zanardi C, Melucci M: **Electrochemical sensing of glucose by chitosan modified graphene oxide.** *J Phys Mater* 2020, **3**, 014011, <https://doi.org/10.1088/2515-7639/ab5e51>.
 14. Shukla SK, Mishra AK, Arotiba OA, Mamba BB: **Chitosan-based nanomaterials: a state-of-the-art review.** *Int J Biol Macromol* 2013, **59**:46–58, <https://doi.org/10.1016/j.jbiomac.2013.04.043>.
 15. Srivastava M, Srivastava SK, Nirala NR, Prakash R: **A chitosan-based polyaniline-Au nanocomposite biosensor for determination of cholesterol.** *Anal. Methods*. 2014, **6**:817–824, <https://doi.org/10.1039/c3ay41812j>.
 16. Wu S, Dai X, Cheng T, Li S: **Highly sensitive and selective ion-imprinted polymers based on one-step electrodeposition of chitosan-graphene nanocomposites for the determination of Cr(VI).** *Carbohydr Polym* 2018, **195**:199–206, <https://doi.org/10.1016/j.carbpol.2018.04.077>.
- For sensitive detection of molecules as small as ions, the functional monomer is a key factor in the interaction process of recognition sites. This paper demonstrates how chitosan can form a highly sensitive material for monitoring of Cr(VI) and compares several electrochemical methods for detection against each other.
17. Jiang Y, Wu J: **Recent development in chitosan nanocomposites for surface-based biosensor applications.** *Electrophoresis* 2019, **40**:2084–2097, <https://doi.org/10.1002/elps.201900066>.
 18. Zouaoui F, Bourouina-Bacha S, Bourouina M, Jaffrezic-Renault N, Zine N, Errachid A: **Electrochemical sensors based on molecularly imprinted chitosan: a review.** *Trends Anal Chem* 2020, **130**:115982, <https://doi.org/10.1016/j.trac.2020.115982>.
- This recent review describes the advances of using chitosan as a functional monomer for Molecularly Imprinted Polymers and highlights its applications in electrochemical sensors. Furthermore, it also gives insight into reagent selection and limitations of the technique.
19. Karrat A, Amine A: **Recent advances in chitosan-based electrochemical sensors and biosensors.** *Arab J Chem Environ Res* 2020, **7**:66–93, <https://doi.org/10.1039/d0tb00569j>.
 20. Qin L, Dong H, Mu Z, Zhang Y, Dong G: **Preparation and bioactive properties of chitosan and casein phosphopeptides composite coatings for orthopedic implants.** *Carbohydr Polym* 2015, **133**:236–244, <https://doi.org/10.1016/j.carbpol.2015.06.099>.
 21. Qin L, Sun H, Hafezi M, Zhang Y: **Polydopamine-assisted immobilization of chitosan brushes on a textured CoCrMo alloy to improve its tribology and biocompatibility.** *Materials* 2019, **12**:3014, <https://doi.org/10.3390/ma12183014>.
 22. Hills KD, Oliveira DA, Cavallaro ND, Gomes CL, McLamore ES: **Actuation of chitosan-aptamer nanobrush borders for pathogen sensing.** *Analyst* 2018, **143**:1650–1661, <https://doi.org/10.1039/c7an02039b>.
 23. Elgadir MA, Uddin MS, Ferdosh S, Adam A, Chowdhury AJK, Sarker MZ: **Impact of chitosan composites and chitosan nanoparticle composites on various drug delivery systems: a review.** *J Food Drug Anal* 2015, **23**:619–629, <https://doi.org/10.1016/j.jfda.2014.10.008>.
 24. Ye Q, Zhou F, Liu W: **Bioinspired catecholic chemistry for surface modification.** *Chem Soc Rev* 2011, **40**:4244–4258, <https://doi.org/10.1039/c1cs15026j>.
 25. Ball V, Del Frari D, Toniazio V, Ruch D: **Kinetics of polydopamine film deposition as a function of pH and dopamine concentration: insights in the polydopamine deposition mechanism.** *J Colloid Interface Sci* 2012, **386**:366–372, <https://doi.org/10.1016/j.jcis.2012.07.030>.
 26. Ryu JH, Messersmith PB, Lee H: **Polydopamine surface chemistry: a decade of discovery.** *ACS Appl Mater Interfaces* 2018, **10**:7523–7540, <https://doi.org/10.1021/acsami.7b19865>.
- This review describes the current state-of-the-art in polydopamine coatings methods and identifies trends in polydopamine research. In particular interest is the discussion on reactivity of the material and what the optimal thickness is for sensor applications.
27. Ju KY, Lee Y, Lee S, Park SB, Lee JK: **Bioinspired polymerization of dopamine to generate melanin-like nanoparticles having an excellent free-radical-scavenging property.** *Bio-macromolecules* 2011, **12**:625–632, <https://doi.org/10.1021/bm101281b>.
 28. Arroquia A, Acosta I, Armada MPG: **Self-assembled gold decorated polydopamine nanospheres as electrochemical sensor for simultaneous determination of ascorbic acid, dopamine, uric acid and tryptophan.** *Mater Sci Eng C* 2020, **109**:110602, <https://doi.org/10.1016/j.msec.2019.110602>.
 29. Li Y, Jiang Y, Song Y, Li Y, Li S: **Simultaneous determination of dopamine and uric acid in the presence of ascorbic acid using a gold electrode modified with carboxylated graphene and silver nanocube functionalized polydopamine nanospheres.** *Microchim Acta* 2018, **185**:382, <https://doi.org/10.1007/s00604-018-2922-3>.
 30. Crapnell RD, Banks CE: **Electroanalytical overview: utilising micro- and nano-dimensional sized materials in electrochemical-based biosensing platforms.** *Microchim Acta* 2021, **188**:268, <https://doi.org/10.1007/s00604-021-04913-y>.
 31. Liu Y, Liang Y, Yang R, Li J, Qu L: **A highly sensitive and selective electrochemical sensor based on polydopamine functionalized graphene and molecularly imprinted polymer for the 2,4-dichlorophenol recognition and detection.** *Talanta* 2019, **195**: 691–698, <https://doi.org/10.1016/j.talanta.2018.11.052>.

32. Lamaoui A, Palacios-Santander JM, Amine A, Cubillana-Aguilera L: **Molecularly imprinted polymers based on polydopamine: assessment of non-specific adsorption.** *Microchem J* 2021, **164**:106043, <https://doi.org/10.1016/j.microc.2021.106043>.
33. Miao J, Liu A, Wu L, Yu M, Wei W, Liu S: **Magnetic ferroferric oxide and polydopamine molecularly imprinted polymer nanocomposites based electrochemical impedance sensor for the selective separation and sensitive determination of dichlorodiphenyltrichloroethane (DDT).** *Anal Chim Acta* 2020, **1095**:82–92, <https://doi.org/10.1016/j.aca.2019.10.027>.
34. Leibl N, Duma L, Gonzato C, Haupt K: **Polydopamine-based molecularly imprinted thin films for electro-chemical sensing of nitro-explosives in aqueous solutions.** *Bioelectrochemistry* 2020, **135**:107541, <https://doi.org/10.1016/j.bioelechem.2020.107541>.
35. Crapnell RD, Hudson A, Foster CW, Eersels K, van Grinsven B, Cleij TJ, Banks CE, Peeters M: **Recent advances in electro-synthesized molecularly imprinted polymer sensing platforms for bioanalyte detection.** *Sensors* 2019, **19**:1204, <https://doi.org/10.3390/s19051204>.
36. Liu K, Wei WZ, Zeng JX, Liu XY, Gao YP: **Application of a novel electrosynthesized polydopamine-imprinted film to the capacitive sensing of nicotine.** *Anal Bioanal Chem* 2006, **385**:724–729, <https://doi.org/10.1007/s00216-006-0489-z>.
37. Tretjakov A, Syritski V, Reut J, Boroznjak R, Volobujeva O, Öpik A: **Surface molecularly imprinted polydopamine films for recognition of immunoglobulin G.** *Microchim Acta* 2013, **180**:1433–1442, <https://doi.org/10.1007/s00604-013-1039-y>.
38. Kanyong P, Rawlinson S, Davis J: **Fabrication and electro-chemical characterization of polydopamine redox polymer modified screen-printed carbon electrode for the detection of guanine.** *Sensor Actuator B Chem* 2016, **233**:528–534, <https://doi.org/10.1016/j.snb.2016.04.099>.
39. Zhang W, Tang Y, Liu J, Ma Y, Jiang L, Huang W, Huo FW, Tian D: **An electrochemical sensor for detecting triglyceride based on biomimetic polydopamine and gold nanocomposite.** *J Mater Chem B* 2014, **2**:8490–8495, <https://doi.org/10.1039/c4tb01439a>.
40. Salgado R, del Valle MA, Duran BG, Pardo MA, Armijo F: **Optimization of dopamine determination based on nanowires PEDOT/polydopamine hybrid film modified electrode.** *J Appl Electrochem* 2014, **44**:1289–1294, <https://doi.org/10.1007/s10800-014-0728-5>.
41. Kim S, Jang LK, Jang M, Lee S, Hardy JG, Lee JY: **Electrically conductive polydopamine-polypyrrole as high performance biomaterials for cell stimulation in vitro and electrical signal recording in vivo.** *ACS Appl Mater Interfaces* 2018, **10**:33032–33042, <https://doi.org/10.1021/acsami.8b11546>.
42. Xu Z, Han R, Liu N, Gao F, Luo X: **Electrochemical biosensors for the detection of carcinoembryonic antigen with low fouling and high sensitivity based on copolymerized polydopamine and zwitterionic polymer.** *Sensor Actuator B Chem* 2020, **319**:128253, <https://doi.org/10.1016/j.snb.2020.128253>.
 This article describes a novel strategy where polydopamine is used to attach sensor recognition elements (in this case aptamers) to another polymer with anti-fouling properties, thus developing a superior sensor for an important cancer biomarker. This opens the field to developing hybrid sensor systems that have superior performance and affinity for target molecules of interest.
43. Lee H, Dellatore SM, Miller WM, Messersmith PB: **Mussel-Inspired surface chemistry for multifunctional coatings.** *Science* 2007, **318**:426–430, <https://doi.org/10.1126/science.1147241>.
 This was the first paper that described and developed polydopamine. The inspiration came from the interest in replicating and understanding the mussel adhesive properties, where one of the proteins was rich in dopamine units and led to follow up work on dopamine polymerization.
44. a Khumsap T, Bamrungsap S, Thu VT, Nguyen LT: **Epitope-imprinted polydopamine electrochemical sensor for ovalbumin detection.** *Bioelectrochemistry* 2021, **140**:107805, <https://doi.org/10.1016/j.bioelechem.2021.107805>.
 b Feng T, Ji W, Zhang Y, Wu F, Tang Q, Wei H, Mao L, Zhang M: **Zwitterionic polydopamine engineered interface for in vivo sensing with high biocompatibility.** *Angew Chem Int Ed* 2020, **59**:23445–23449, <https://doi.org/10.1002/anie.202010675>.
45. Aguilar-Ferrer D, Szweczyk J, Coy E: **Recent developments in polydopamine-based photocatalytic nanocomposites for energy production: physico-chemical properties and perspectives.** *Catal Today* 2021, <https://doi.org/10.1016/j.cattod.2021.08.016>.